



User Manual

Refractometer PCE-010 / PCE-018 / PCE-032 / PCE-4582 / PCE-5890 / PCE-Oe / PCE-SG / PCE-ALK
/ PCE-0100



User manuals in various languages (français, italiano, español, português, nederlands, türk, polski, русский, 中文) can be found by using our product search on: www.pce-instruments.com

Last change: 25 February 2022
v1.0



Contents

| | | |
|----------|--------------------------------|----------|
| 1 | Safety notes | 1 |
| 2 | Operation | 2 |
| 3 | Technical data | 2 |
| 4 | Scope of delivery | 3 |
| 5 | Evaluation | 3 |
| 6 | Calibration | 5 |
| 7 | Contact | 5 |
| 8 | Disposal | 5 |

1 Safety notes

Please read this manual carefully and completely before you use the device for the first time. The device may only be used by qualified personnel and repaired by PCE Instruments personnel. Damage or injuries caused by non-observance of the manual are excluded from our liability and not covered by our warranty.

- The device must only be used as described in this instruction manual. If used otherwise, this can cause dangerous situations for the user and damage to the meter.
- The instrument may only be used if the environmental conditions (temperature, relative humidity, ...) are within the ranges stated in the technical specifications. Do not expose the device to extreme temperatures, direct sunlight, extreme humidity or moisture.
- Do not expose the device to shocks or strong vibrations.
- The case should only be opened by qualified PCE Instruments personnel.
- Never use the instrument when your hands are wet.
- You must not make any technical changes to the device.
- The appliance should only be cleaned with a damp cloth. Use only pH-neutral cleaner, no abrasives or solvents.
- The device must only be used with accessories from PCE Instruments or equivalent.
- Before each use, inspect the case for visible damage. If any damage is visible, do not use the device.
- Do not use the instrument in explosive atmospheres.
- The measurement range as stated in the specifications must not be exceeded under any circumstances.
- Non-observance of the safety notes can cause damage to the device and injuries to the user.

We do not assume liability for printing errors or any other mistakes in this manual.

We expressly point to our general guarantee terms which can be found in our general terms of business.

If you have any questions please contact PCE Instruments. The contact details can be found at the end of this manual.



2 Operation




At the beginning of the measuring procedure, carefully clean the hinged lid and the prism and then dry them. Now place 1-2 drops of the sample on the prism. When closing the hinged lid, the sample is evenly distributed between the lid and the prism. To put the sample on the main prism, you can use the pipette. Make sure that no air bubbles form as this would negatively affect the measurement result. By moving the hinged lid slightly, the sample liquid can be distributed evenly. Now hold the refractometer against bright daylight. You can now see the scale through the eyepiece. The value is read between the light / dark border. By turning the eyepiece, you can focus the scale if necessary. To prevent deposits from forming on the prism and the lid, the device should be carefully cleaned and dried after each measuring process.

Refractometers work according to the principle of light refraction. With these devices, you can easily and accurately determine the concentration of e. g. starch, glues, adhesives..., the mixing ratio of liquid media and the sugar content of milk, juice, wine.... Thus, the devices can be used in many industries as a quick measuring instrument in production and laboratories. All models have automatic temperature compensation (ATC).

- Simply coat the prism with the liquid to be measured.
- Read the concentration value on the optical scale.
- Automatic temperature compensation ATC
- Robust metal housing
- Supplied with pipette, screwdriver, case

3 Technical data

| Models | PCE-010 | PCE-018 | PCE-032 | PCE-4582 PCE-5890 | PCE-Oe |
|--------------------|--|---|--|--------------------------------------|---------------------|
| Meas. range | 0 ... 10 % Brix | 0 ... 18 % Brix | 0 ... 32 % Brix | 45 ... 82 % Brix 58 ... 90 % Brix | 0 ... 140 ° Oechsle |
| Accuracy | 0.1 % | 0.1 % | 0.2 % | 0.5 % | 2 ° Oe |
| Resolution | 0.1 % | 0.1 % | 0.2 % | 0.5 % | 2 ° Oe |
| Applications | Fruit, juices, oils, cutting compounds, lubricants | Fruit juices, soft drinks, beer, mixed drinks | Emulsions, starches, glues, mulled wines | Viscous juices, condensed milk, jams | Wines |
| Temperature comp.. | 10 ... 30 °C | 10 ... 30 °C | 10 ... 30 °C | 10 ... 30 °C | 10 ... 30 °C |
| Display | | | | | |
| Dimensions | 200 x Ø29mm | 200 x Ø29mm | 172 x Ø29mm | 147 x Ø29mm | 172 x Ø29mm |
| Weight | 280g | 280g | 260g | 240g | 260g |

| Models | PCE-0100 | PCE-ALK | PCE-SG |
|--------------------|---|---|--|
| Meas. range | 0 ... 100 % salt content | 0 ... 80 % vol. | 0 °C ... 50 °C coolant / antifreeze 0 °C ... -40 °C cleaning agent 1.15 - 1.30 SG battery acid content |
| Accuracy | 0.001 | 1 % | ± 5 °C antifreeze ± 5 °C detergent ± 0.01 SG battery acid content |
| Resolution | 0.001 % | 1 % (0 ... 60 % vol.) 2% (60 ... 80 vol.) | 5 °C antifreeze 5 °C detergent 0.01 SG battery acid content |
| Applications | Salinity | Alcoholic beverages | Lubricants, coolants, antifreeze, cleaning agents, battery acid content |
| Temperature comp.. | 10 ... 30 °C | 10 ... 30 °C | 10 ... 30 °C |
| Display |  |  |  |
| Dimensions | 200 x Ø29mm | 203 x Ø29mm | 157 x Ø29mm |
| Weight | 300g | 280g | 230g |

4 Scope of delivery

Refractometer, pipette, adjusting screwdriver, care cloth, instructions, case

5 Evaluation

Evaluation of the alcohol content in must by refractometry

With the refractometer, you can indirectly determine the potential alcohol content by determining the sugar content of the must.

The higher the sugar content of a must, the higher its density. This means that the light beam has a slower velocity and endures a deviation. This deviation depends on the sugar concentration and other soluble substances, so that the higher the concentration, the greater the deviation of the incident light beam and vice versa. The refractometer allows to check the relationship between the refractive index and the sugar concentration in different units of measure by the correct use of graduated scales. The main unit of measurement displayed on the refractometer is Brix (° Brix) or per cent in sucrose. You have to take into account that the temperature has an influence on the sample. Therefore, you have to use a temperature correction to be able to measure under regular temperature, the European standard is 20 °C. Our refractometers do not need a temperature correction because they include an automatic temperature compensation and all values are measured below 20 °C.

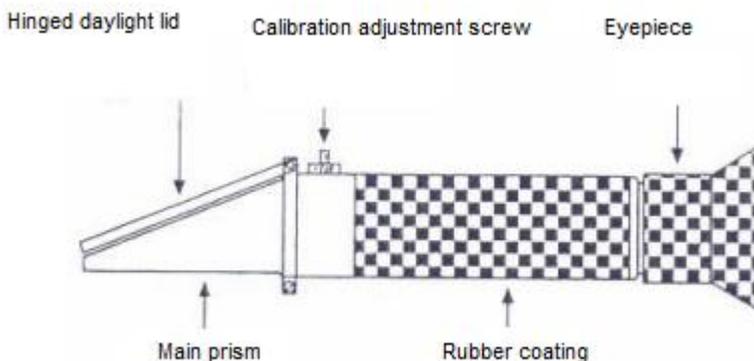


Before you use the device, it must be calibrated. The sample must be prepared by filtering the must. The first drops are discarded (to use our refractometers, the temperature of the sample must be within a range of 20 ... 30 °C and must never exceed 30 °C). Now place 1 - 2 drops of the sample on the prism. By moving the hinged lid slightly, the sample liquid can be distributed evenly. Two measurements should be made.

After having the result in Brix (per cent in sucrose), you can calculate the alcohol content with the help of a formula (valid for the range 15 ... 25 Brix):

$$\% \text{ vol} = (0.6757 \times \text{°Brix}) - 2.0839$$

or you can use the chart below, especially when the range is exceeded.



EXAMPLE:

With our refractometer, we measured a sample with a sugar concentration of 24.2° Brix. If we do not have any charts and want to determine the alcohol content, we have to apply the formula:

$$\% \text{ vol} = (0.6757 \times 24.2^\circ) - 2.0839 = 16.35 - 2.0839 = 14.31 \% \text{ vol}$$

If we have charts, we can look for the reading **24.2°** in the first column and get the corresponding value of alcohol content in the last column. In our example for **24.2° Brix**, the alcohol content is **14.28 % vol**.

6 Calibration

Before calibration, carefully clean and dry the instrument. Now add 1-2 drops of distilled water to the prism. If the light / dark limit is not at 0 % (water line), this must be adjusted via the calibration screw under the rubber cover, using the screwdriver supplied. The PCE-4582 and PCE 5890 cannot be calibrated with distilled water, a sample solution with a known sugar content (e. g. 70 % sugar solution) should be used.

Note:

Instruments are already calibrated at the factory.

Important notes:

- The hinged lid and the prism should be kept clean at all costs; dirt will impair the measuring accuracy.
- Avoid scratches on the prism and the hinged lid, this also has a negative influence on the measurement.
- Do not use any sharp, aggressive cleaning agents for cleaning but only a damp cloth. Dry the meter well afterwards.
- Clean the instrument only with a damp cloth, never under water, as this could penetrate the instrument.
- Prevent shocks and impacts as this can destroy the optics
- Store the instrument in a dry place.

7 Contact

If you have any questions, suggestions or technical problems, please do not hesitate to contact us. You will find the relevant contact information at the end of this user manual.

8 Disposal

For the disposal of batteries in the EU, the 2006/66/EC directive of the European Parliament applies. Due to the contained pollutants, batteries must not be disposed of as household waste. They must be given to collection points designed for that purpose.

In order to comply with the EU directive 2012/19/EU we take our devices back. We either re-use them or give them to a recycling company which disposes of the devices in line with law.

For countries outside the EU, batteries and devices should be disposed of in accordance with your local waste regulations.

If you have any questions, please contact PCE Instruments.





PCE Instruments contact information

Germany

PCE Deutschland GmbH
Im Langel 26
D-59872 Meschede
Deutschland
Tel.: +49 (0) 2903 976 99 0
Fax: +49 (0) 2903 976 99 29
info@pce-instruments.com
www.pce-instruments.com/deutsch

United Kingdom

PCE Instruments UK Ltd
Unit 11 Southpoint Business Park
Ensign Way, Southampton
Hampshire
United Kingdom, SO31 4RF
Tel: +44 (0) 2380 98703 0
Fax: +44 (0) 2380 98703 9
info@pce-instruments.co.uk
www.pce-instruments.com/english

The Netherlands

PCE Brookhuis B.V.
Institutenweg 15
7521 PH Enschede
Nederland
Telefoon: +31 (0)53 737 01 92
info@pcebenelux.nl
www.pce-instruments.com/dutch

France

PCE Instruments France EURL
23, rue de Strasbourg
67250 Soultz-Sous-Forets
France
Téléphone: +33 (0) 972 3537 17
Numéro de fax: +33 (0) 972 3537 18
info@pce-france.fr
www.pce-instruments.com/french

Italy

PCE Italia s.r.l.
Via Pesciatina 878 / B-Interno 6
55010 Loc. Gragnano
Capannori (Lucca)
Italia
Telefono: +39 0583 975 114
Fax: +39 0583 974 824
info@pce-italia.it
www.pce-instruments.com/italiano

United States of America

PCE Americas Inc.
1201 Jupiter Park Drive, Suite 8
Jupiter / Palm Beach
33458 FL
USA
Tel: +1 (561) 320-9162
Fax: +1 (561) 320-9176
info@pce-americas.com
www.pce-instruments.com/us

Spain

PCE Ibérica S.L.
Calle Mayor, 53
02500 Tobarra (Albacete)
España
Tel. : +34 967 543 548
Fax: +34 967 543 542
info@pce-iberica.es
www.pce-instruments.com/espanol

Turkey

PCE Teknik Cihazları Ltd.Şti.
Halkalı Merkez Mah.
Pehlivan Sok. No.6/C
34303 Küçükçekmece - İstanbul
Türkiye
Tel: 0212 471 11 47
Faks: 0212 705 53 93
info@pce- cihazlari.com.tr
www.pce-instruments.com/turkish